

FIG. 1

2

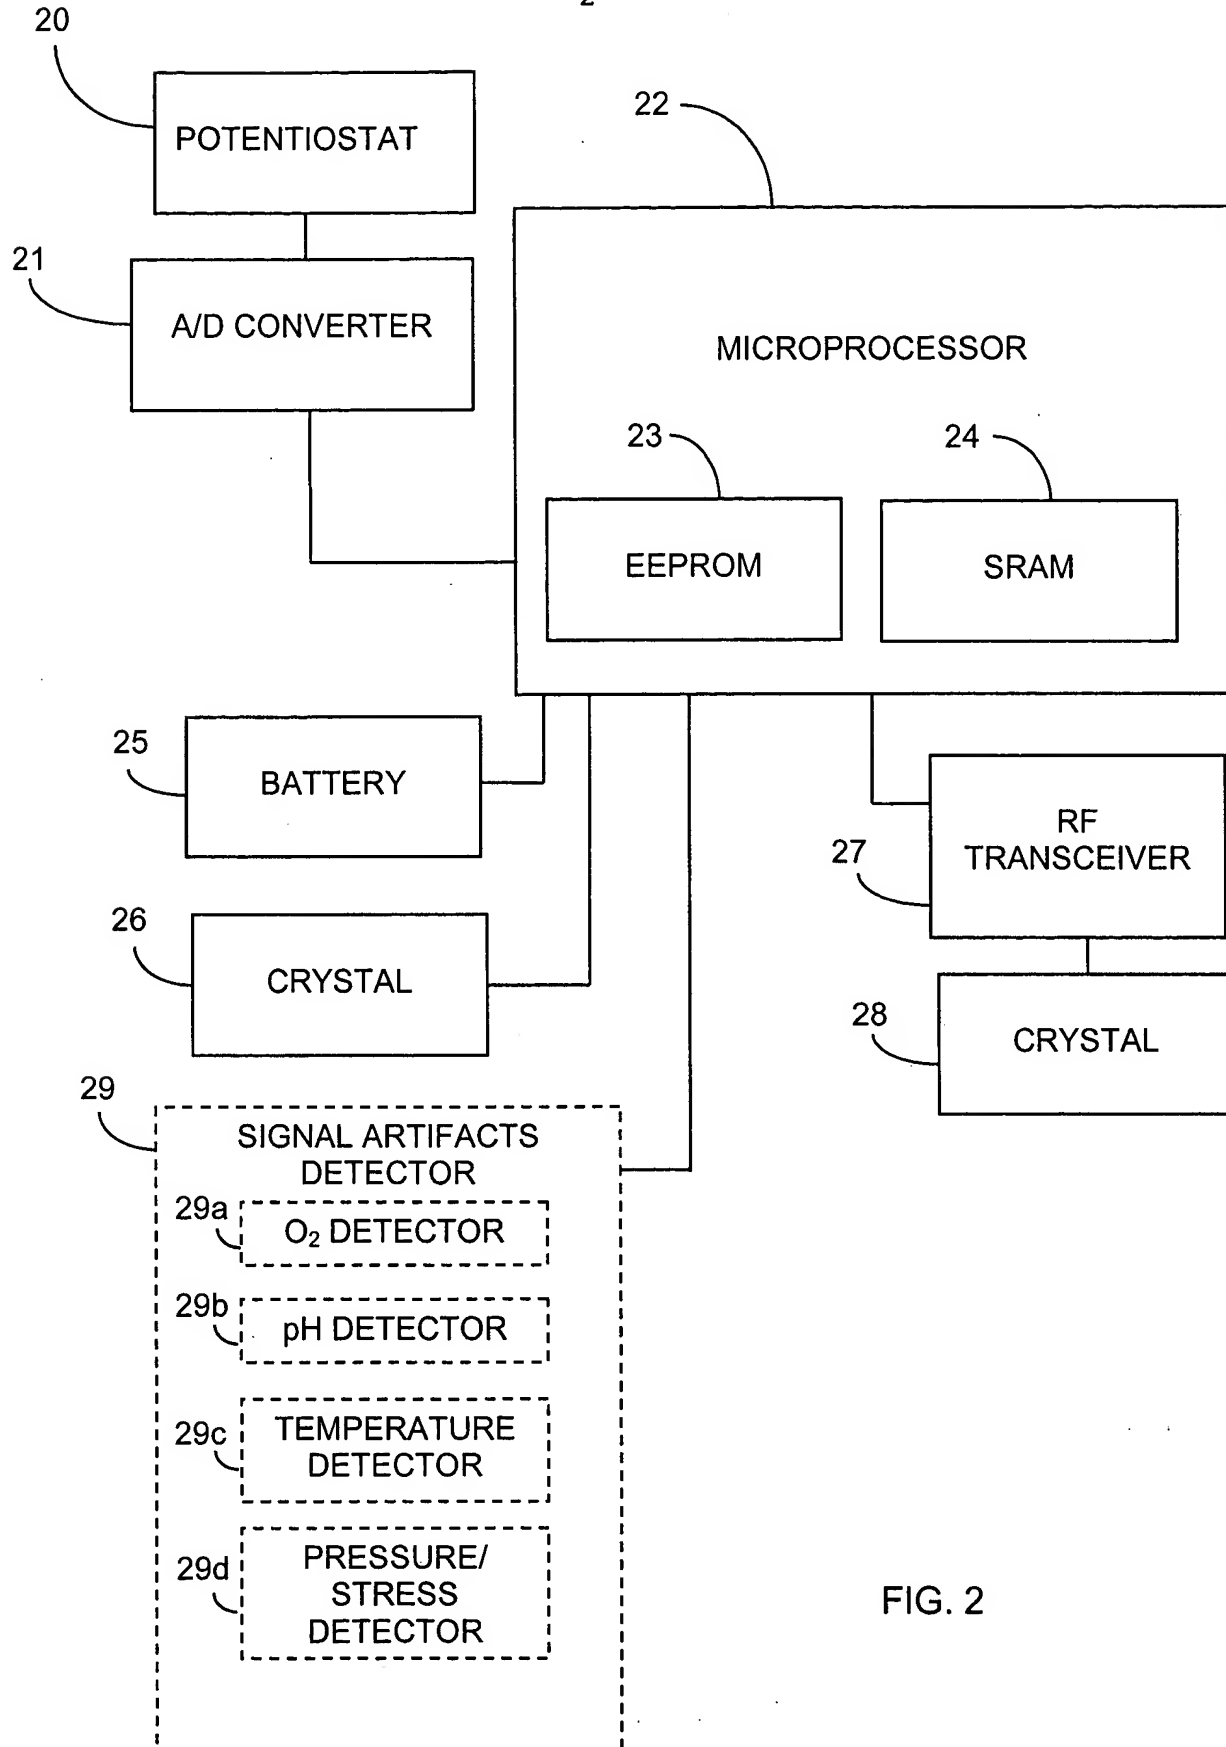


FIG. 2

3

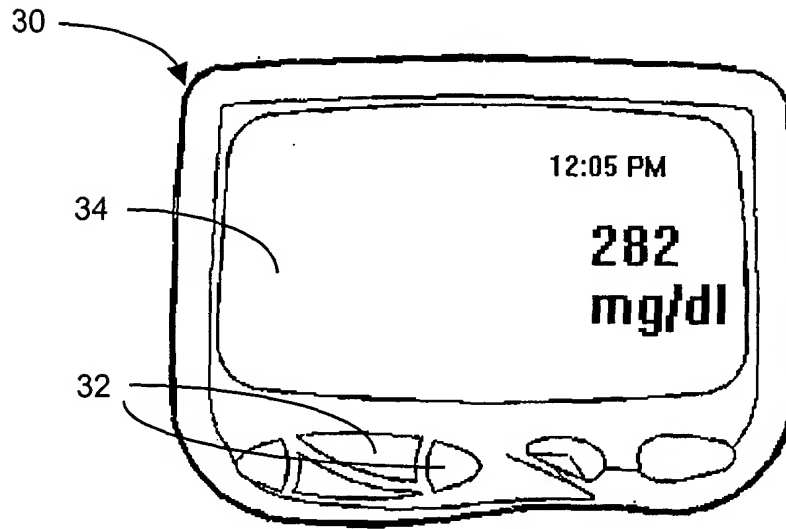


FIG. 3A

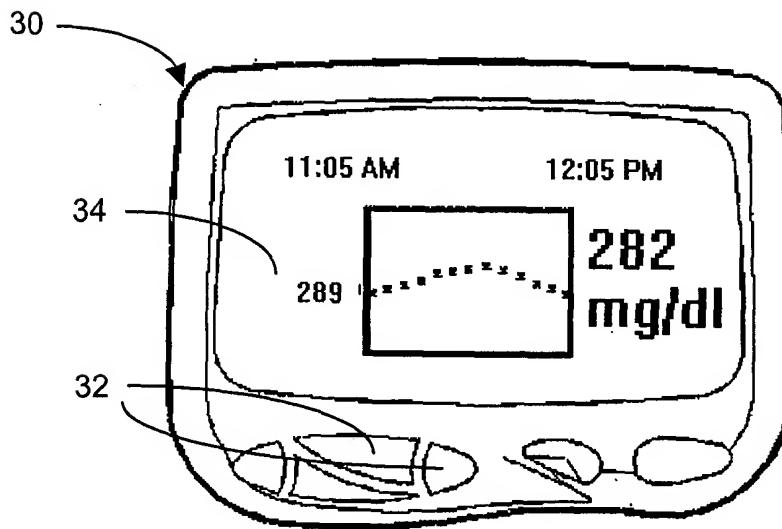


FIG. 3B

SYSTEMS AND METHOD FOR REPLACING SIGNAL ARTIFACTS IN A  
GLUCOSE SENSOR DATA STREAM

Goode, et al.

Appl. No.: Unknown Atty Docket: DEXCOM.027A

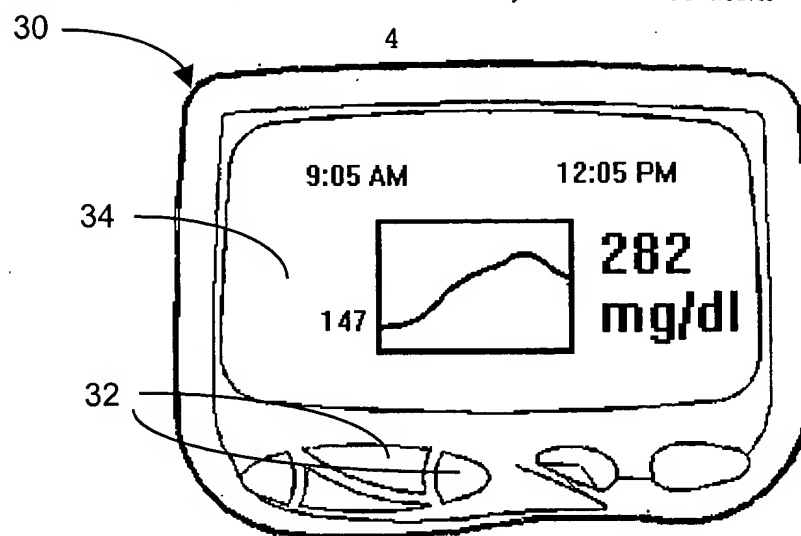


FIG. 3C

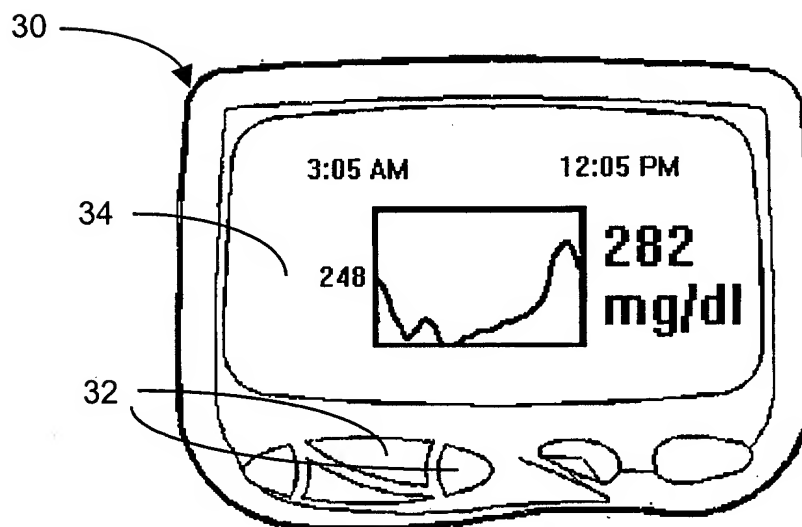


FIG. 3D

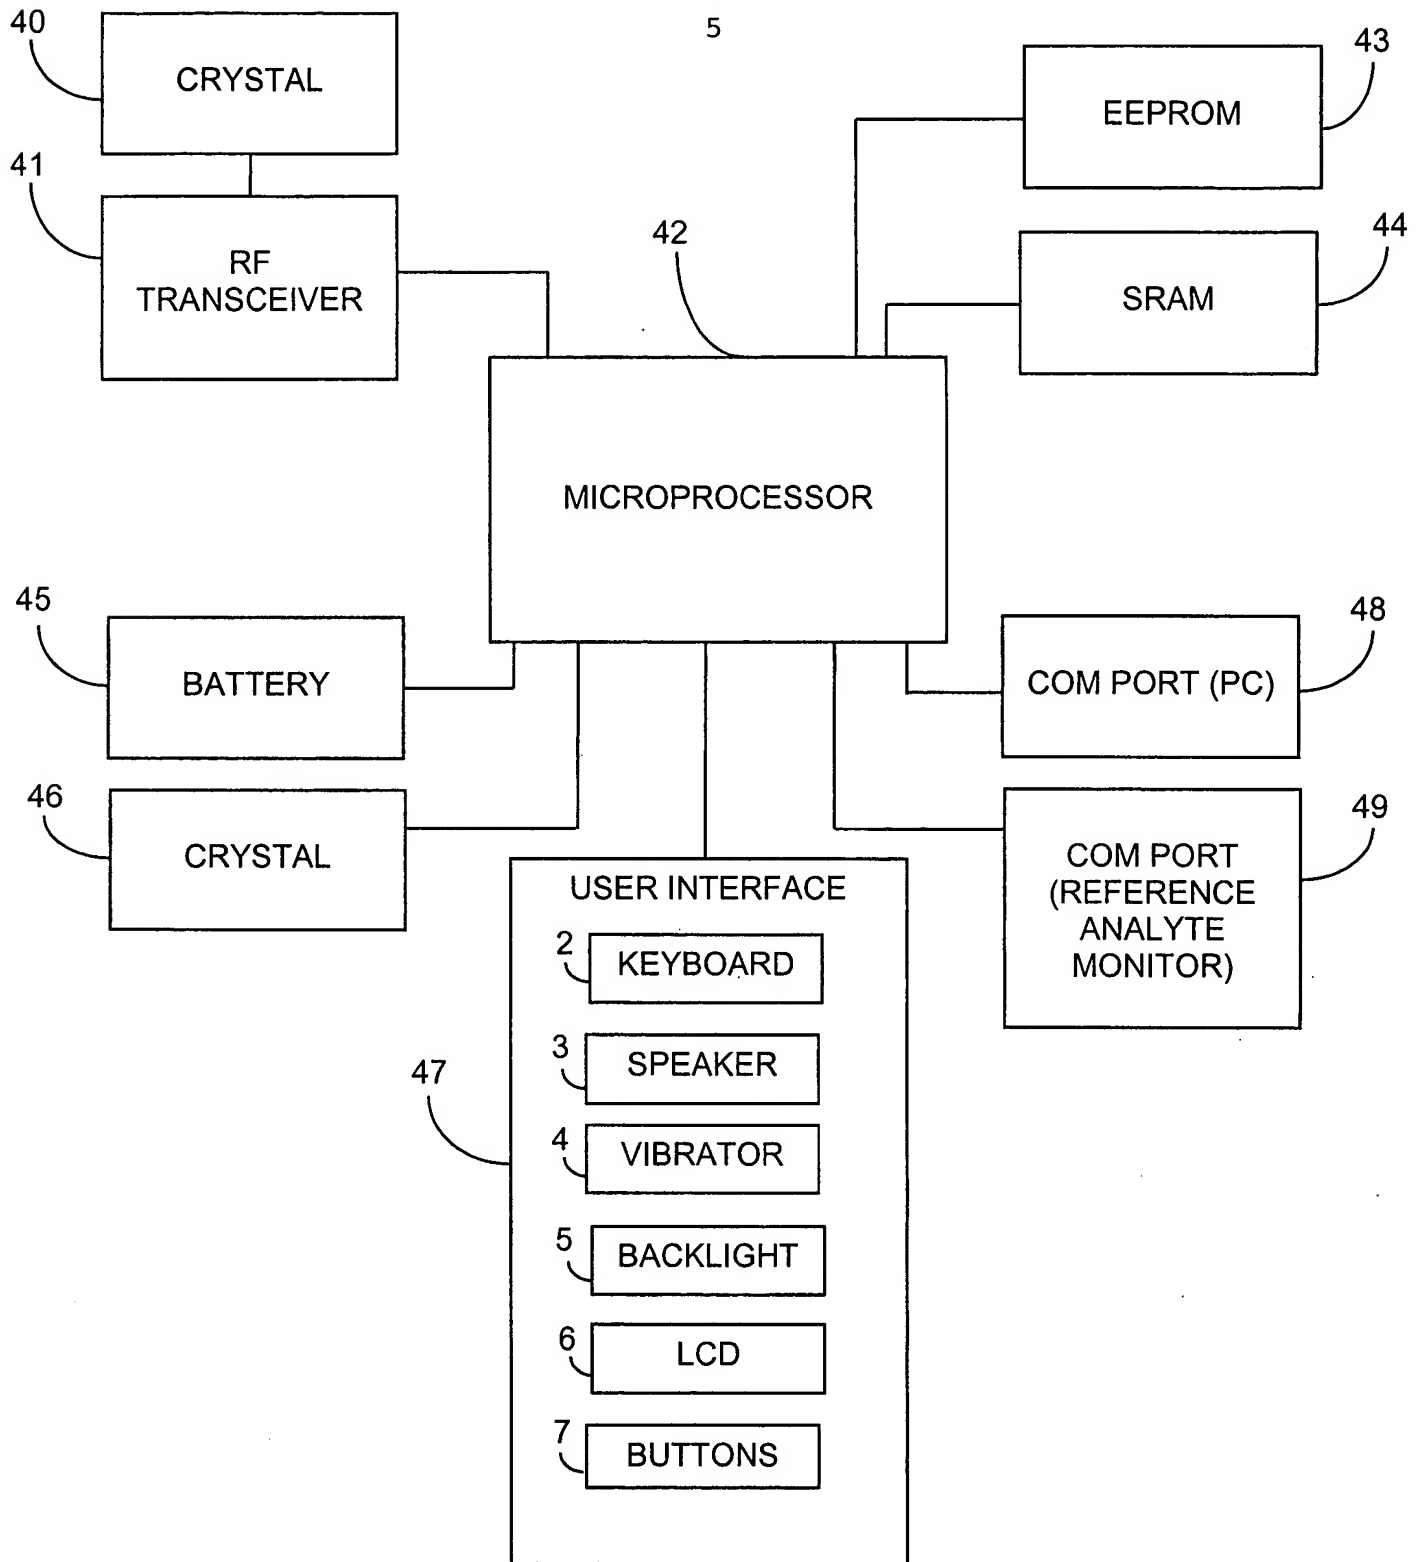


FIG. 4

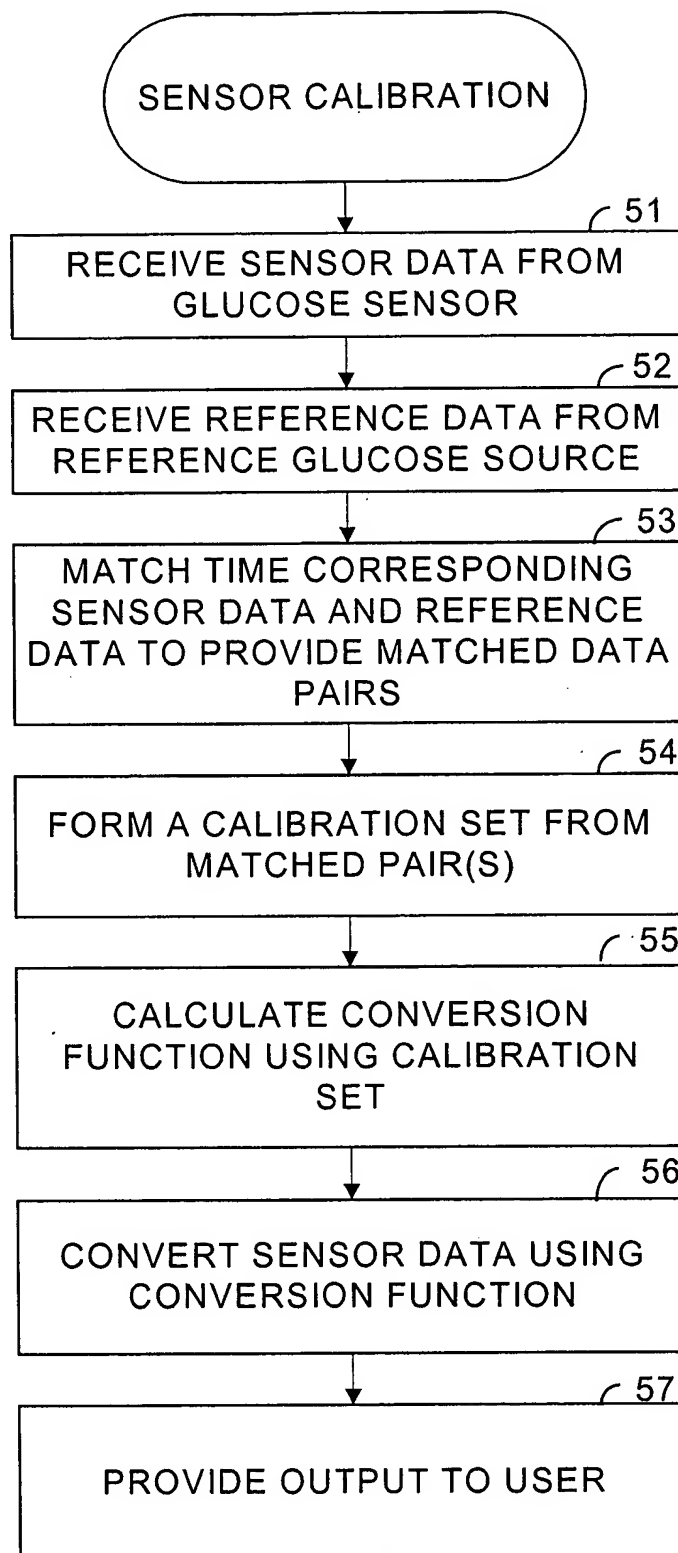


FIG. 5

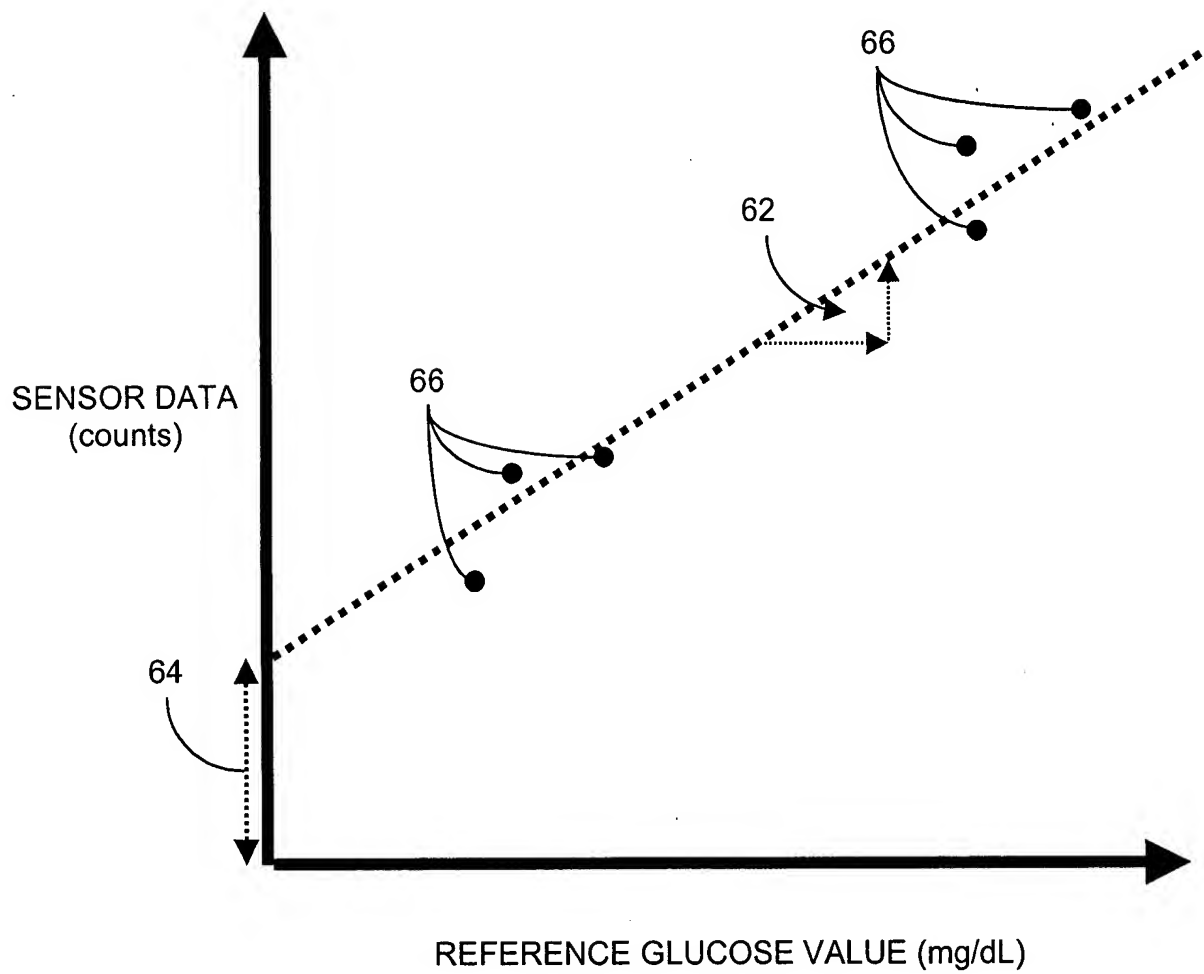


FIG. 6

SYSTEMS AND METHOD FOR REPLACING SIGNAL ARTIFACTS IN A  
GLUCOSE SENSOR DATA STREAM

Goode, et al.

Appl. No.: Unknown

Atty Docket: DEXCOM.027A

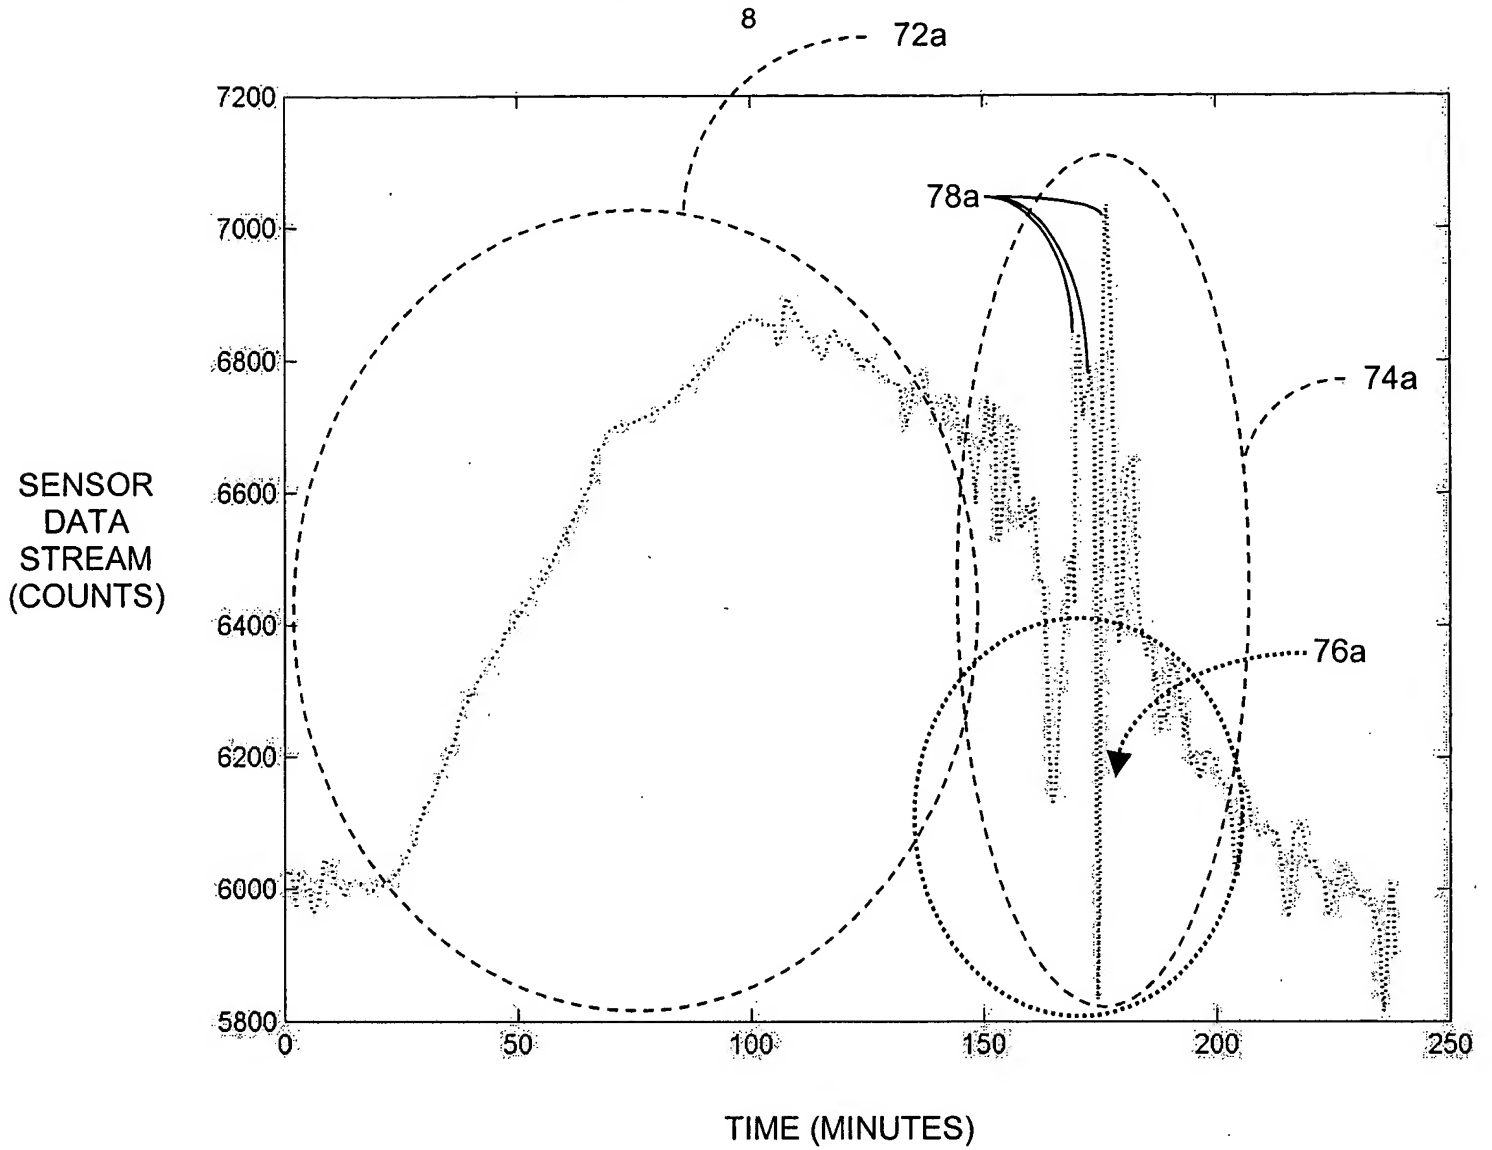


FIG. 7A



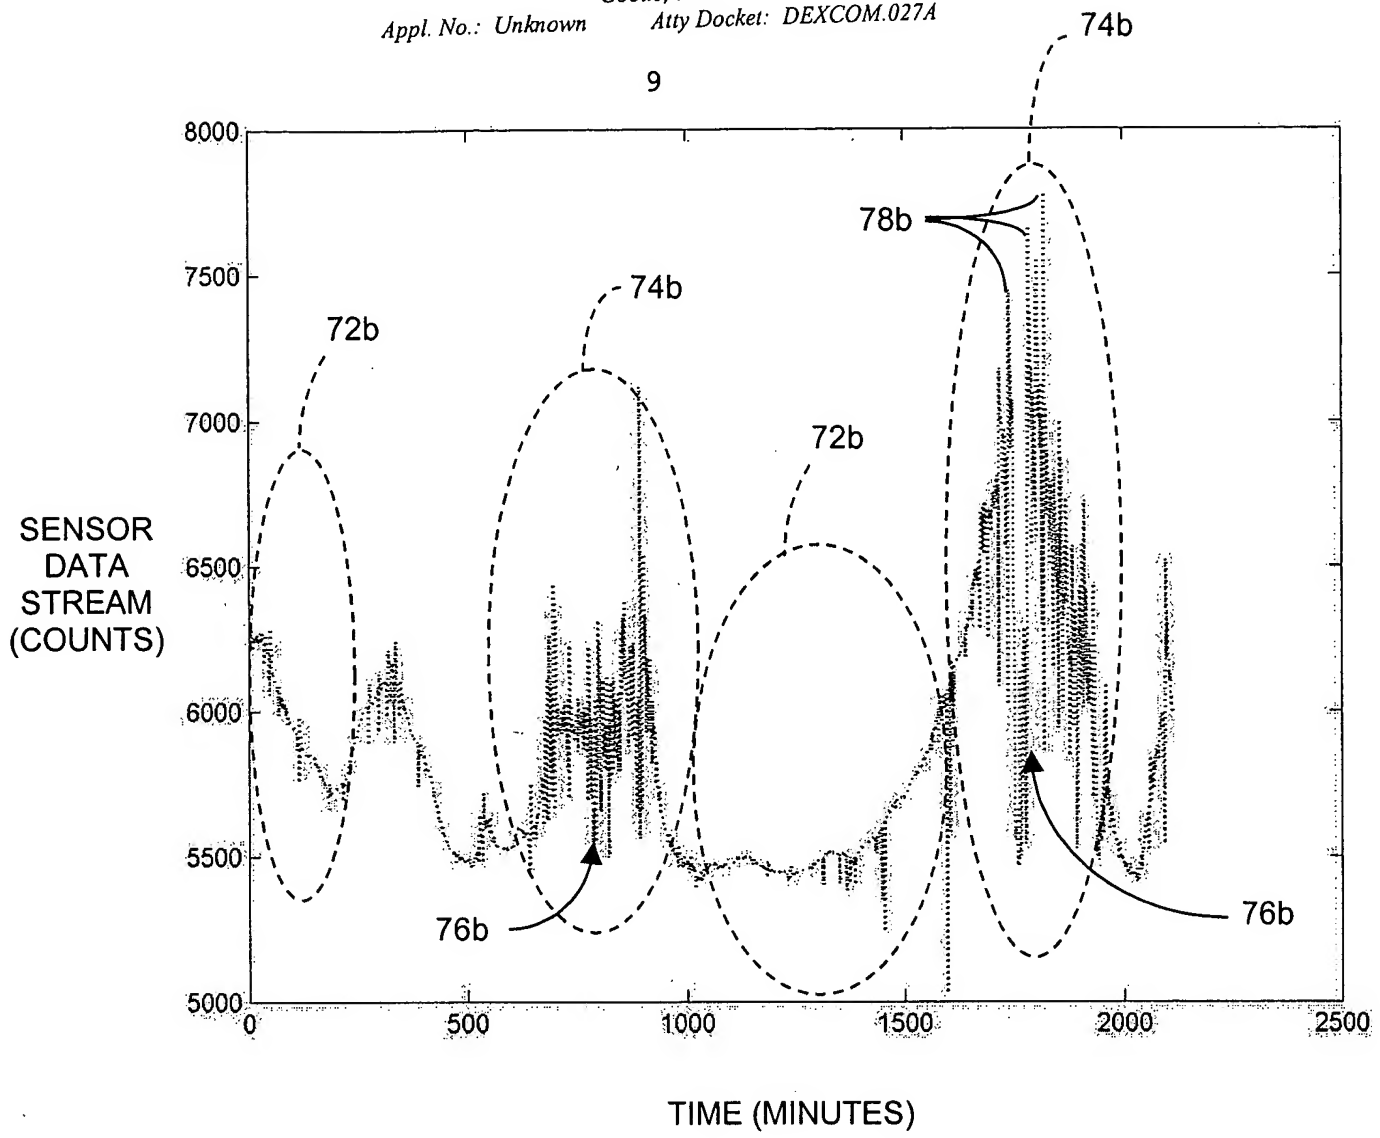


FIG. 7B

10

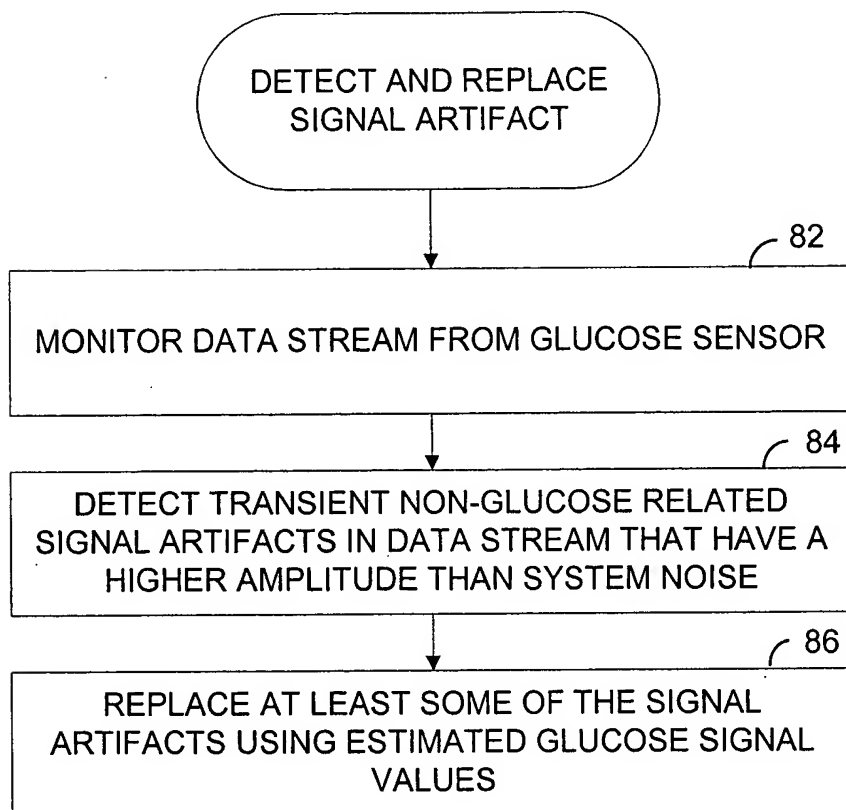


FIG. 8

SYSTEMS AND METHOD FOR REPLACING SIGNAL ARTIFACTS I  
GLUCOSE SENSOR DATA STREAM

Goode, et al.

Appl. No.: Unknown Atty Docket: DEXCOM.027A

11

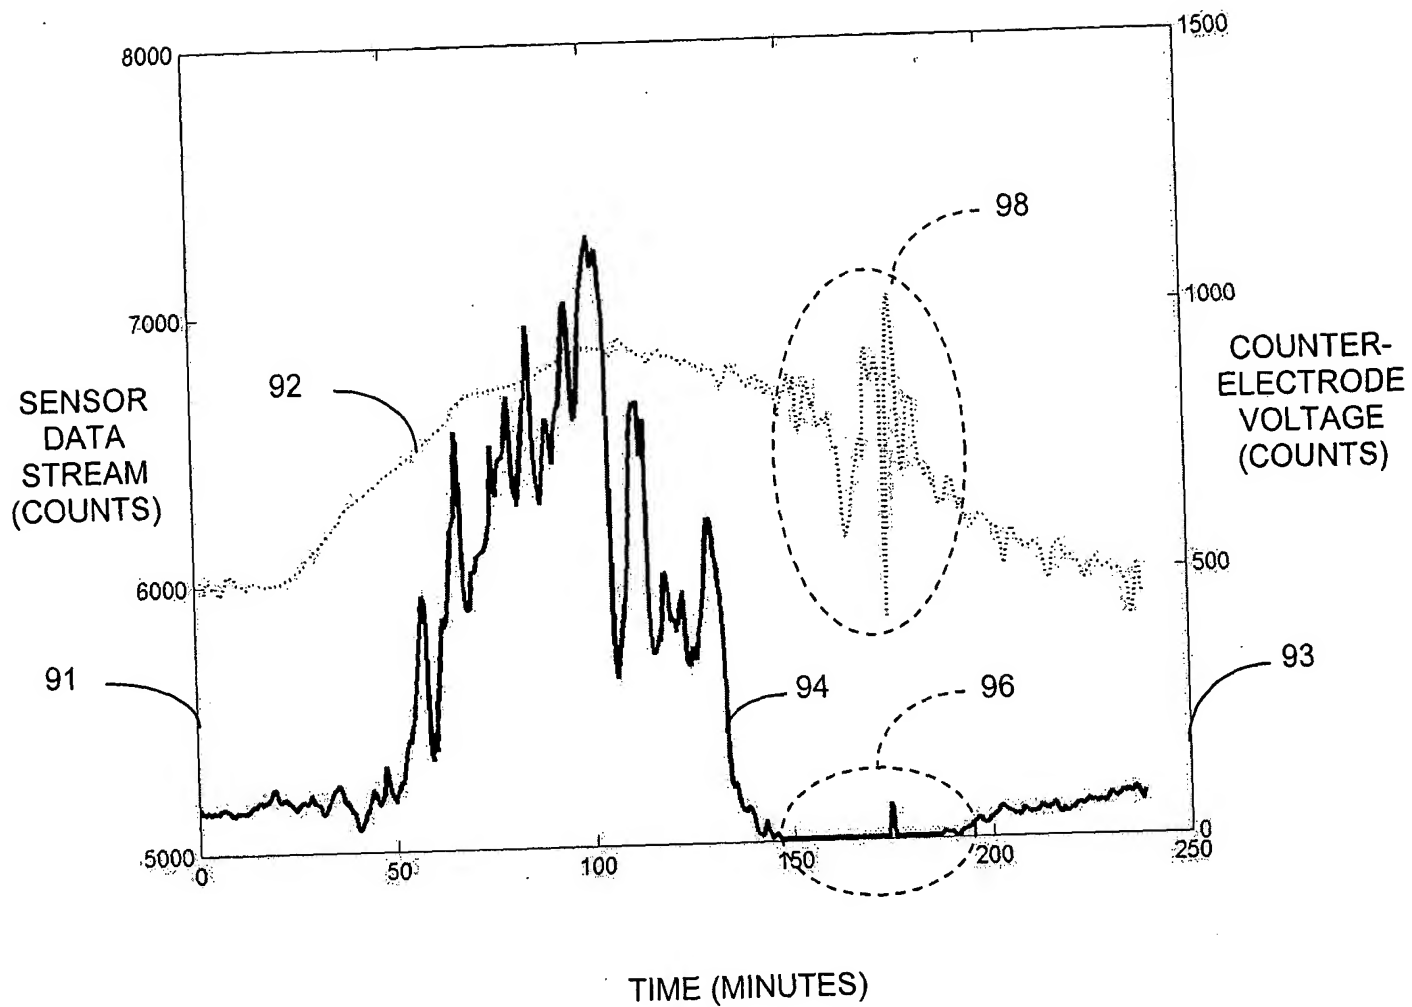


FIG. 9

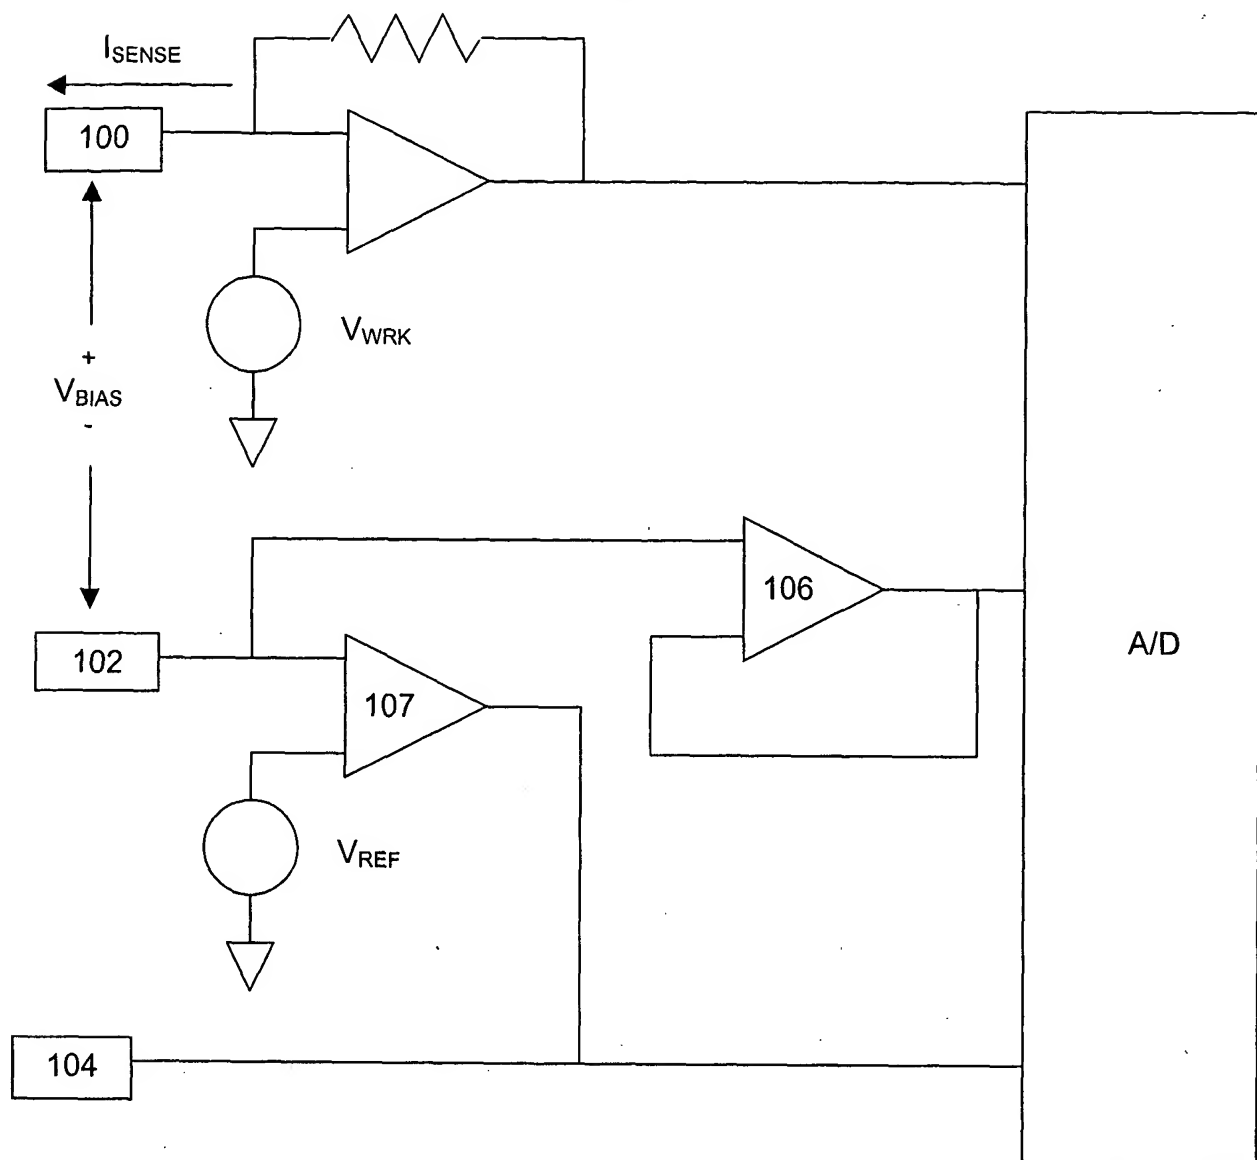


FIG. 10A

SYSTEMS AND METHOD FOR REPLACING SIGNAL ARTIFACTS I  
GLUCOSE SENSOR DATA STREAM

Goode, et al.

Appl. No.: Unknown

Atty Docket: DEXCOM.027A

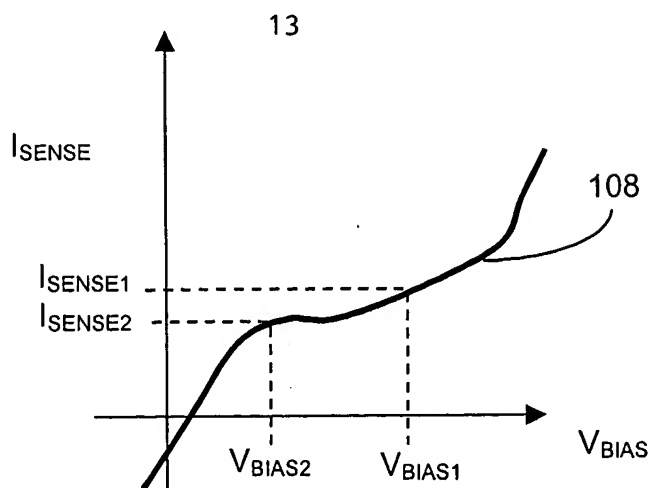


FIG. 10B

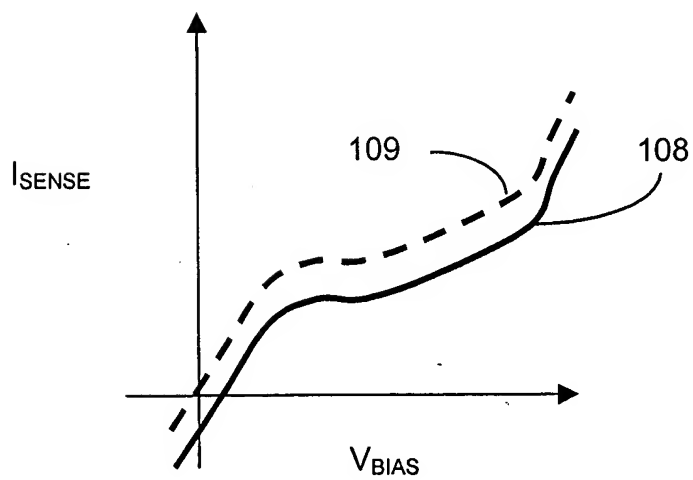


FIG. 10C

SYSTEMS AND METHOD FOR REPLACING SIGNAL ARTIFACTS IN  
GLUCOSE SENSOR DATA STREAM

Goode, et al.

Appl. No.: Unknown Atty Docket: DEXCOM.027A

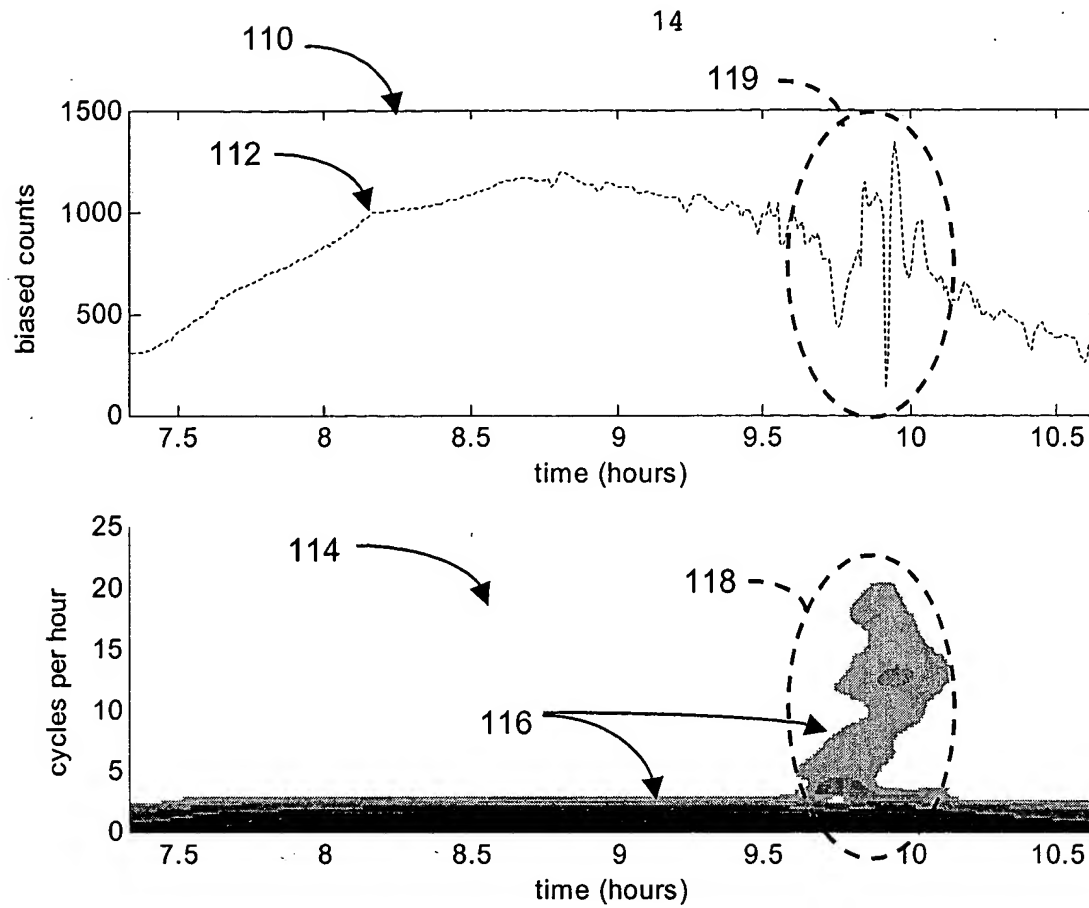


FIG. 11

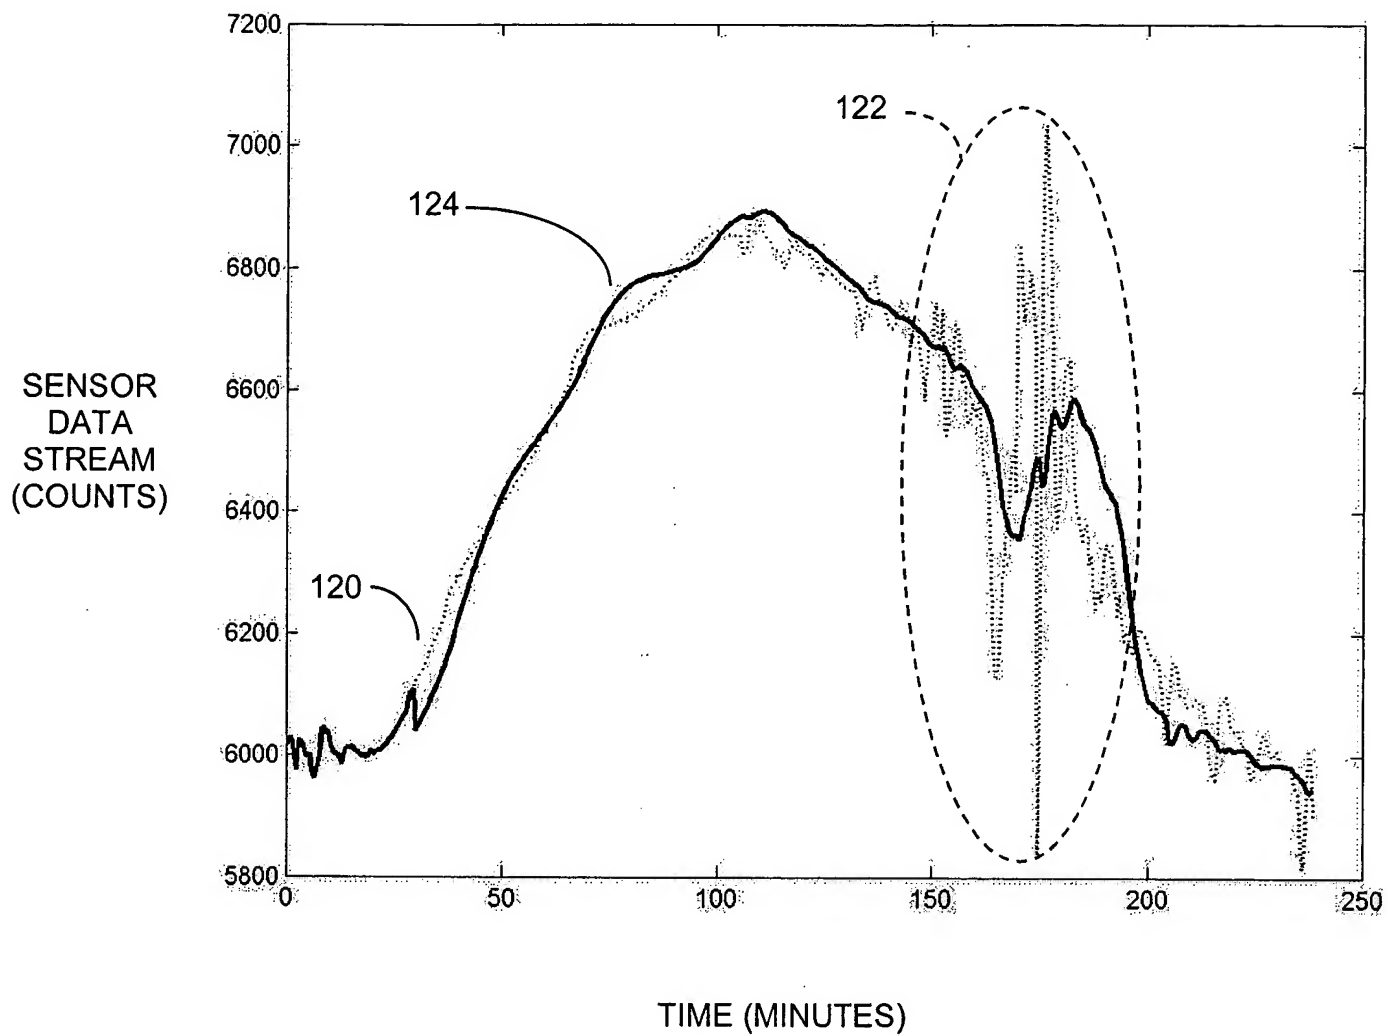


FIG. 12

SYSTEMS AND METHOD FOR REPLACING SIGNAL ARTIFACTS I  
GLUCOSE SENSOR DATA STREAM

Goode, et al.

Appl. No.: Unknown Atty Docket: DEXCOM.027A

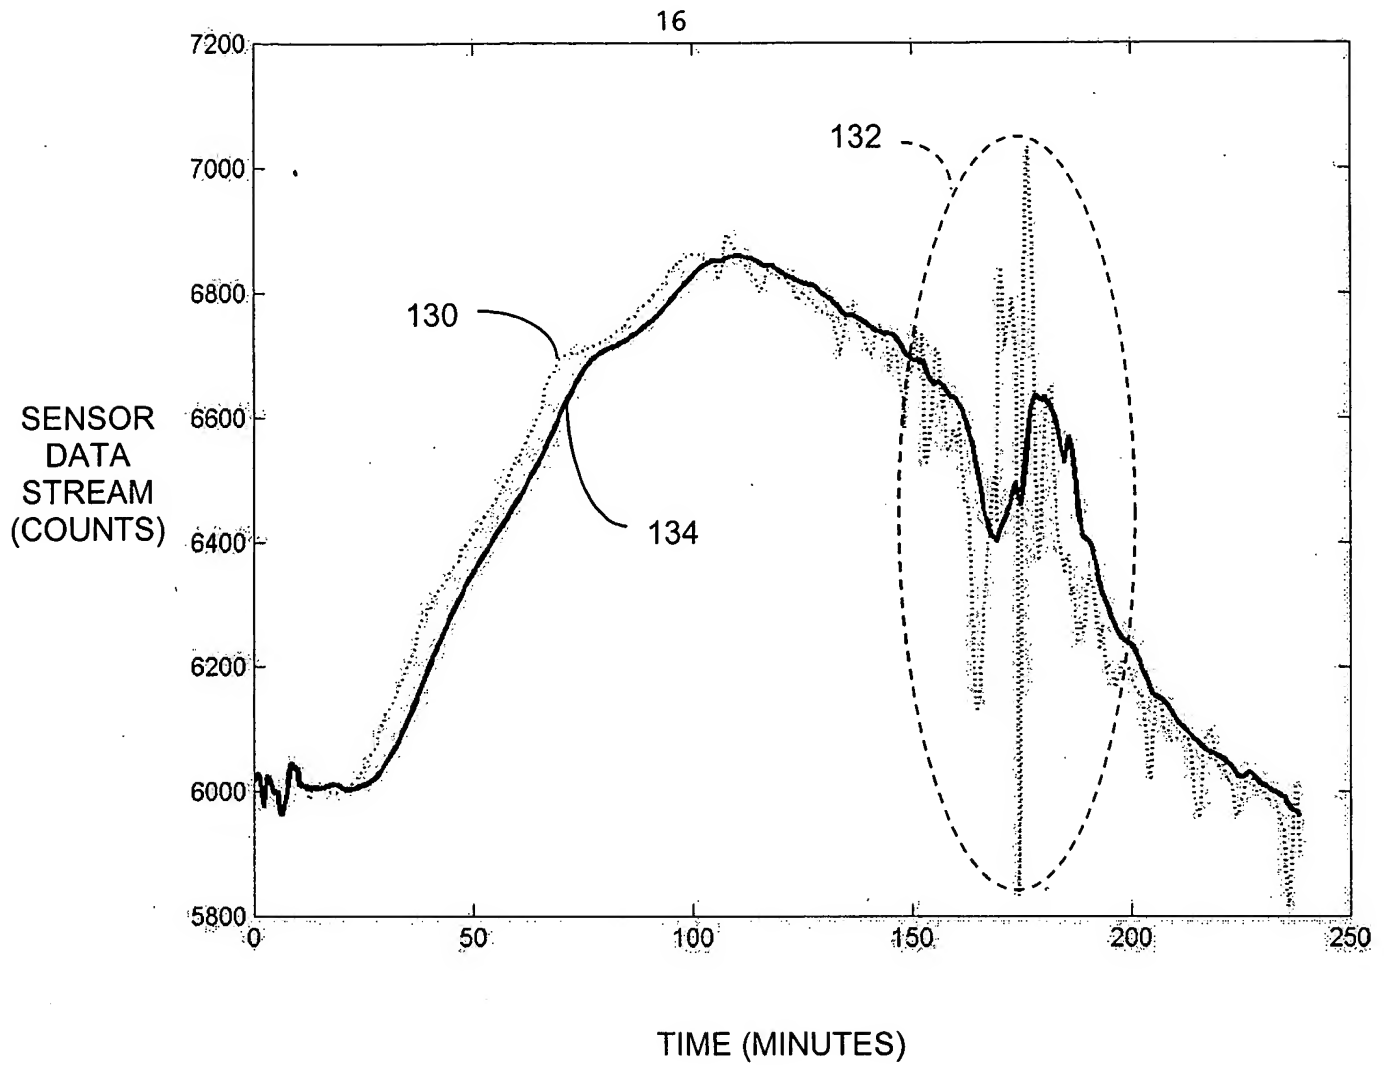


FIG. 13



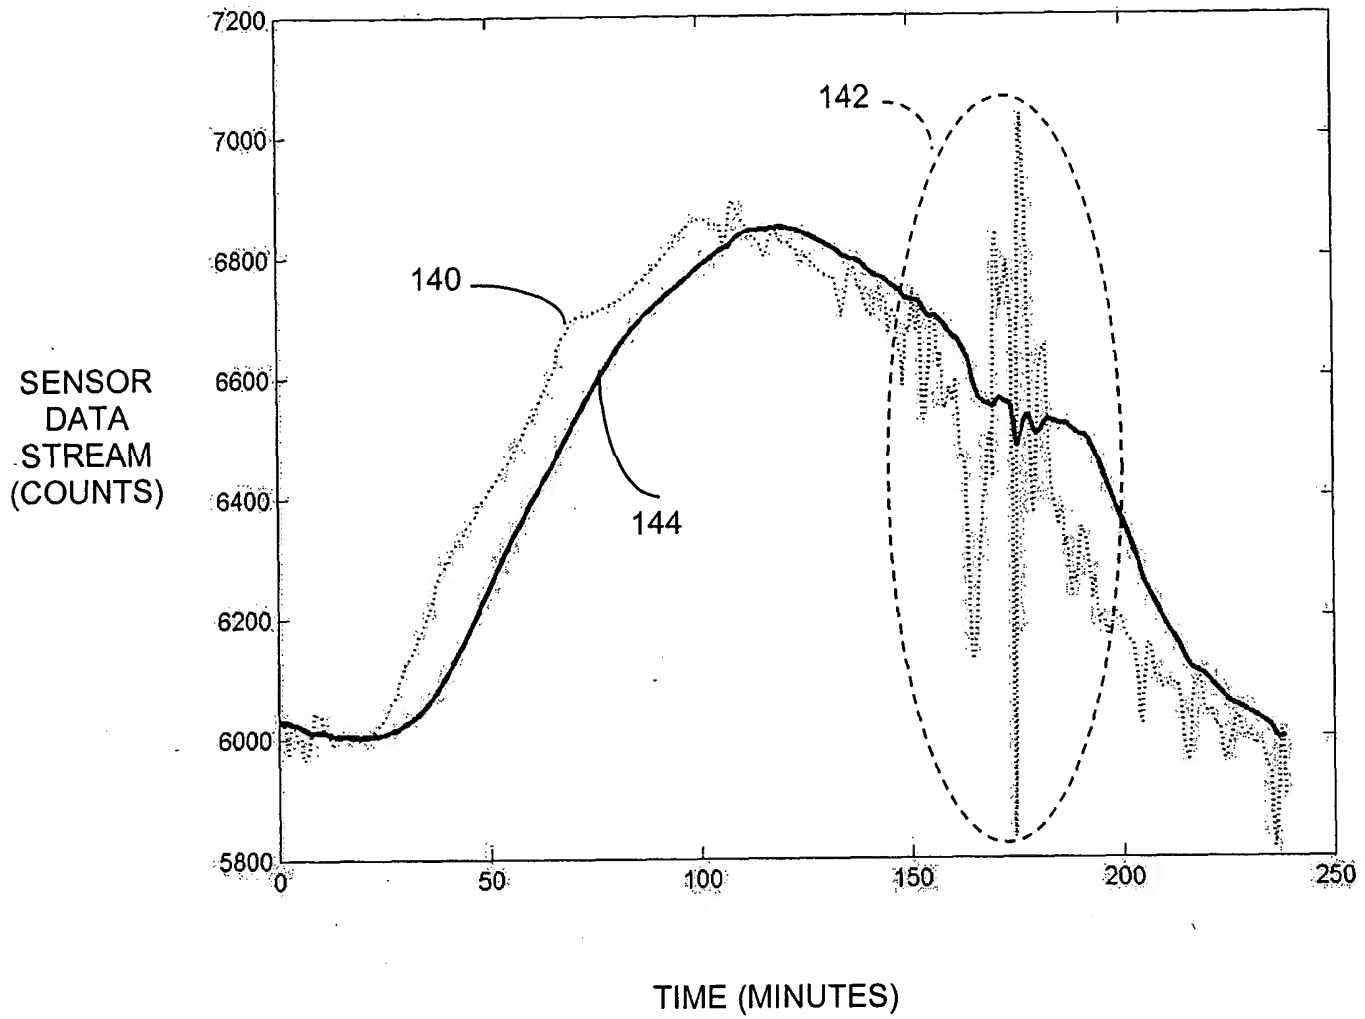


FIG. 14

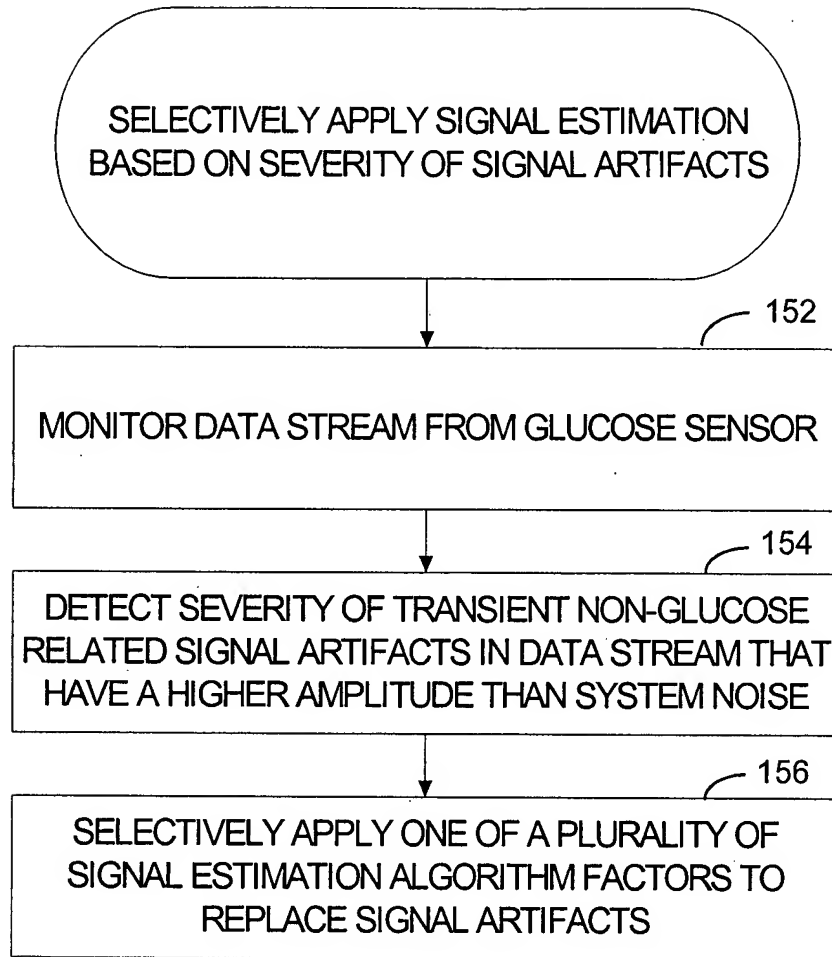


FIG. 15

SYSTEMS AND METHOD FOR REPLACING SIGNAL ARTIFACTS I  
GLUCOSE SENSOR DATA STREAM

Goode, et al.

Appl. No.: Unknown Atty Docket: DEXCOM.027A

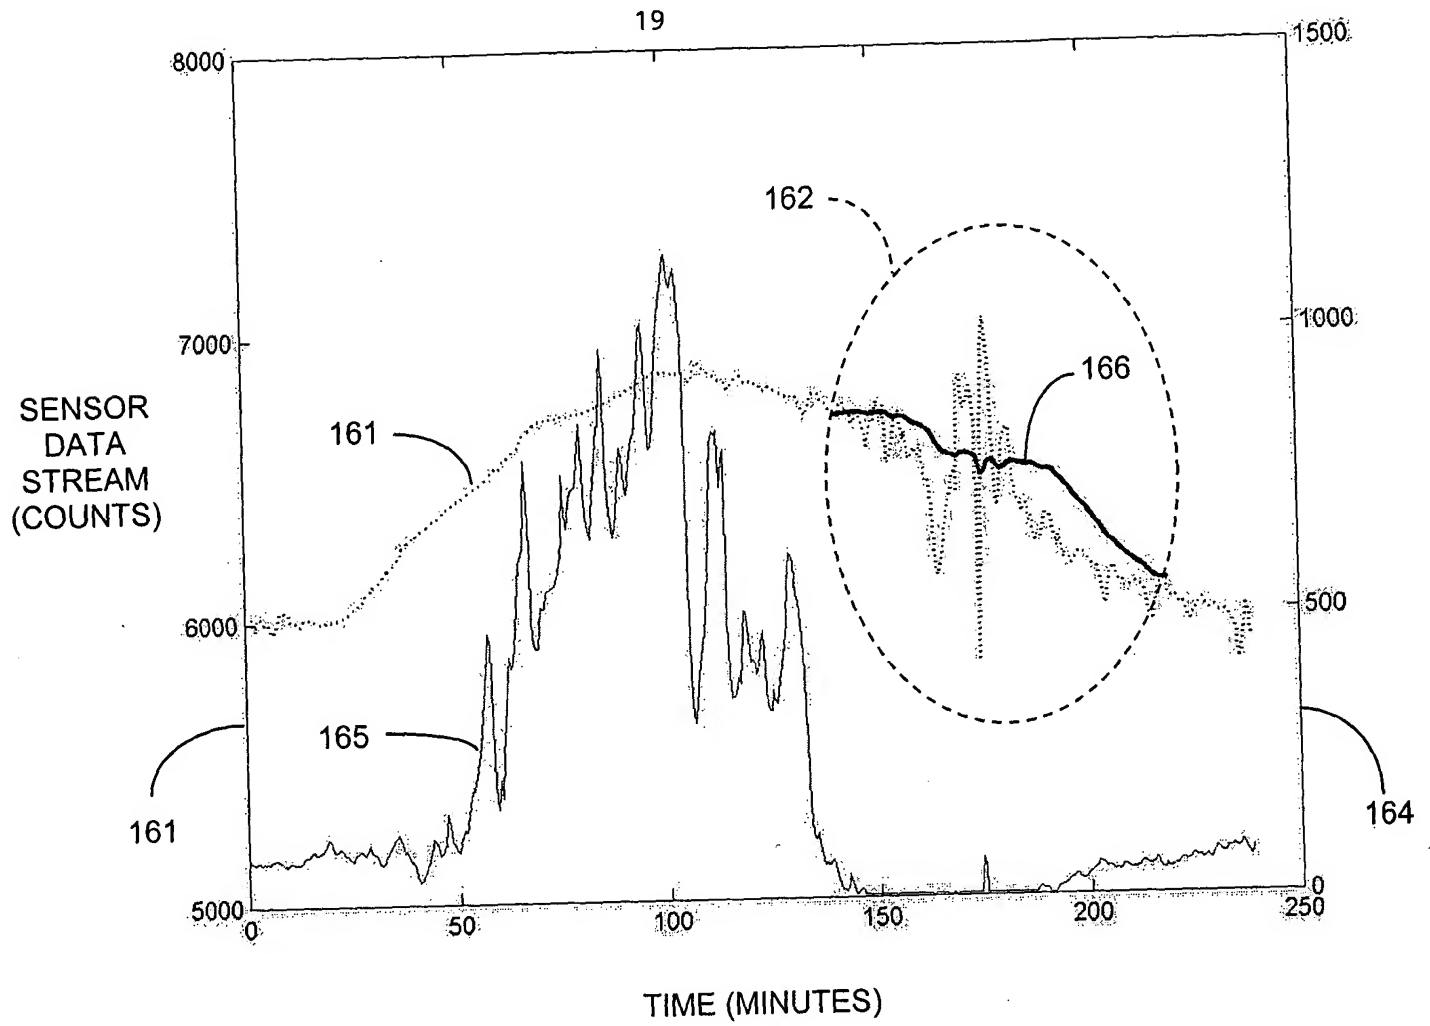


FIG. 16

SYSTEMS AND METHOD FOR REPLACING SIGNAL ARTIFACTS I  
GLUCOSE SENSOR DATA STREAM

Goode, et al.

Appl. No.: Unknown Atty Docket: DEXCOM.027A

20

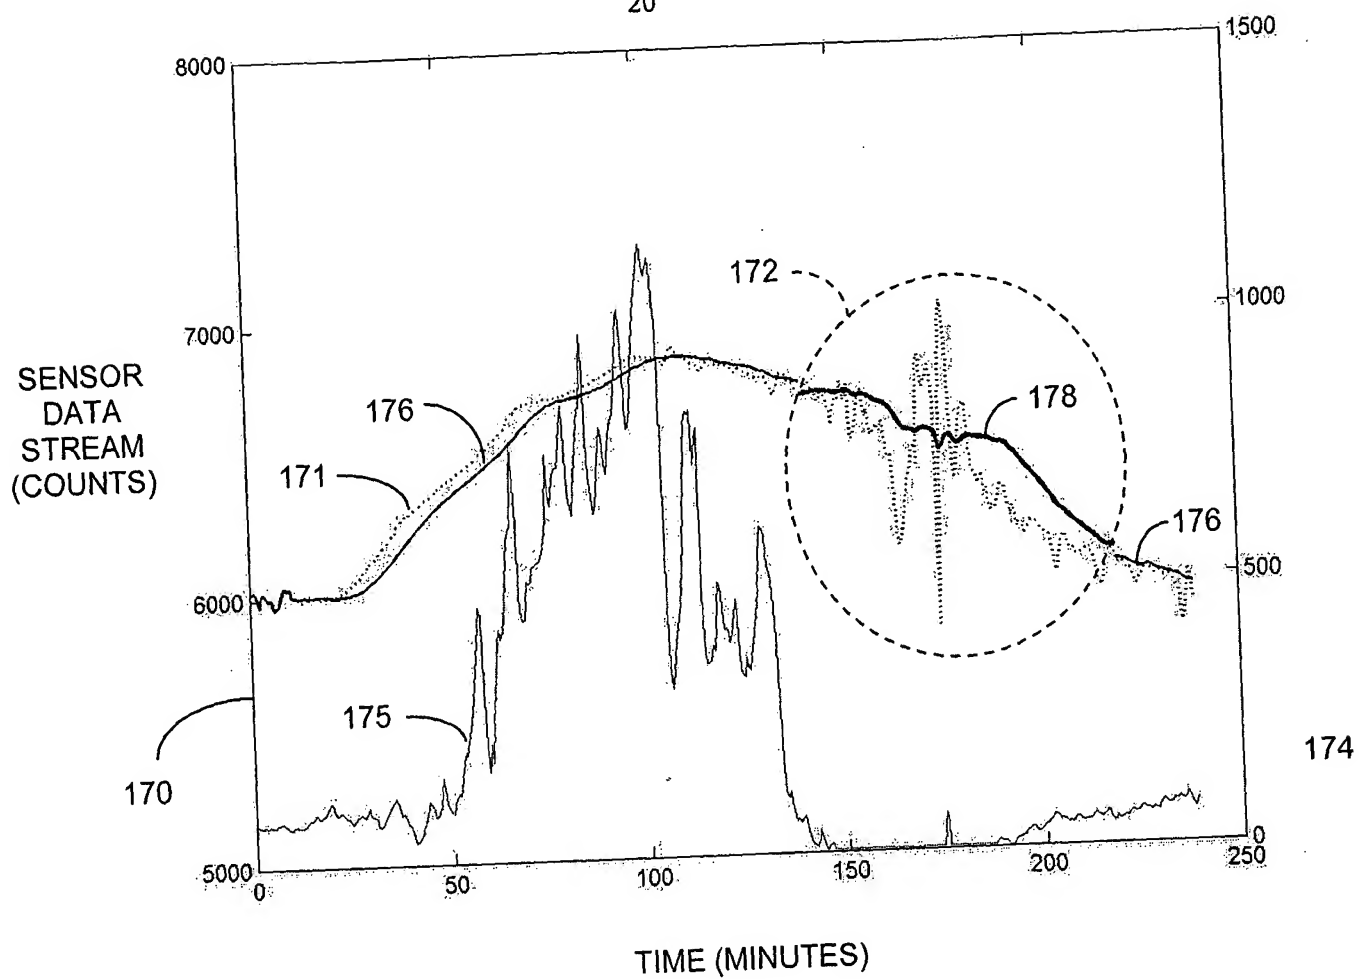


FIG. 17